



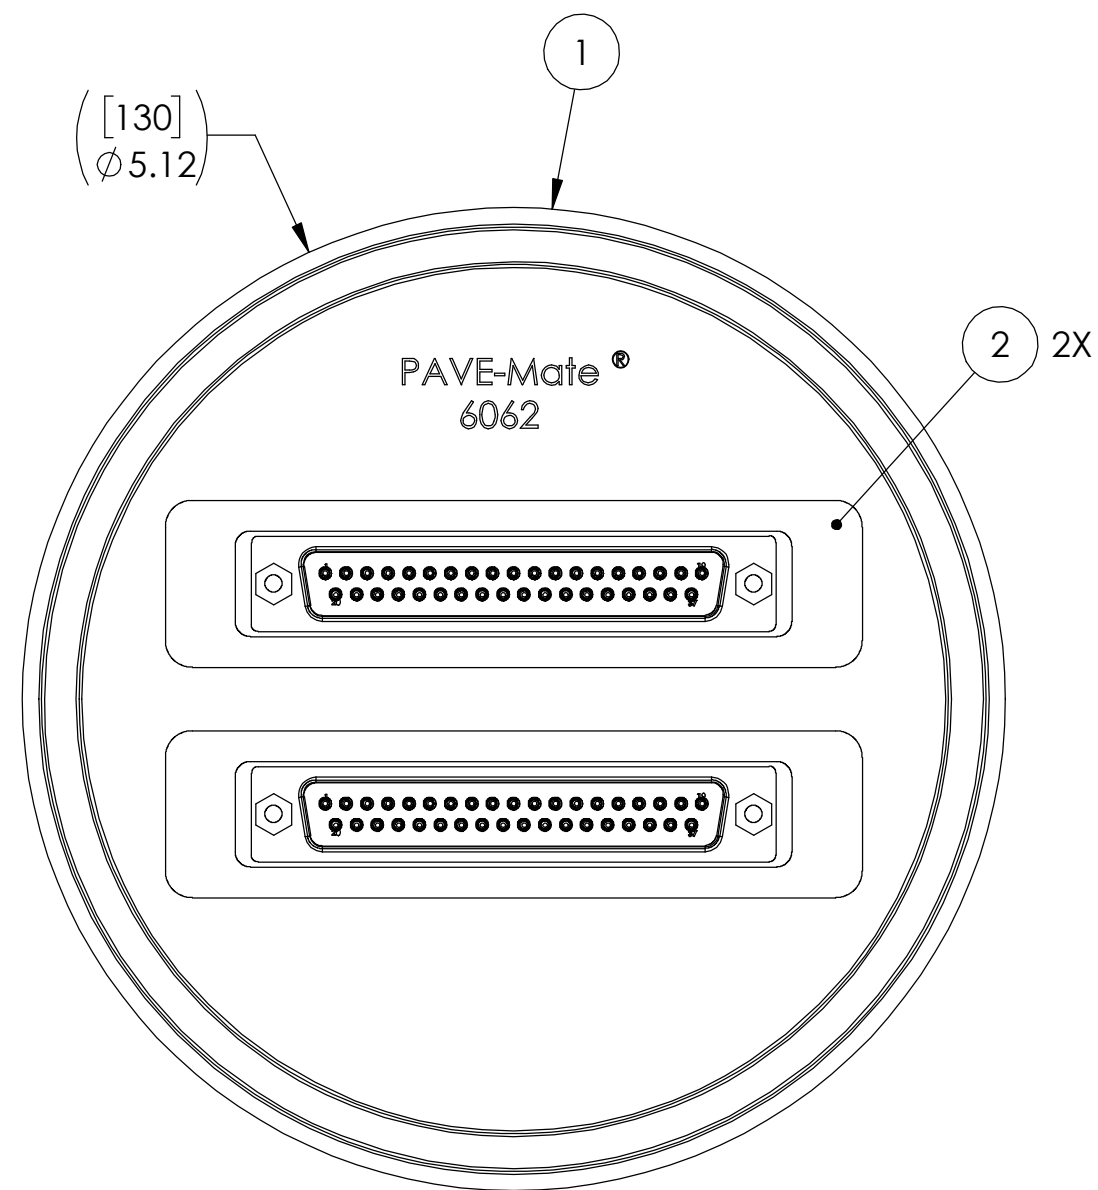

ATMOSPHERE | VACUUM

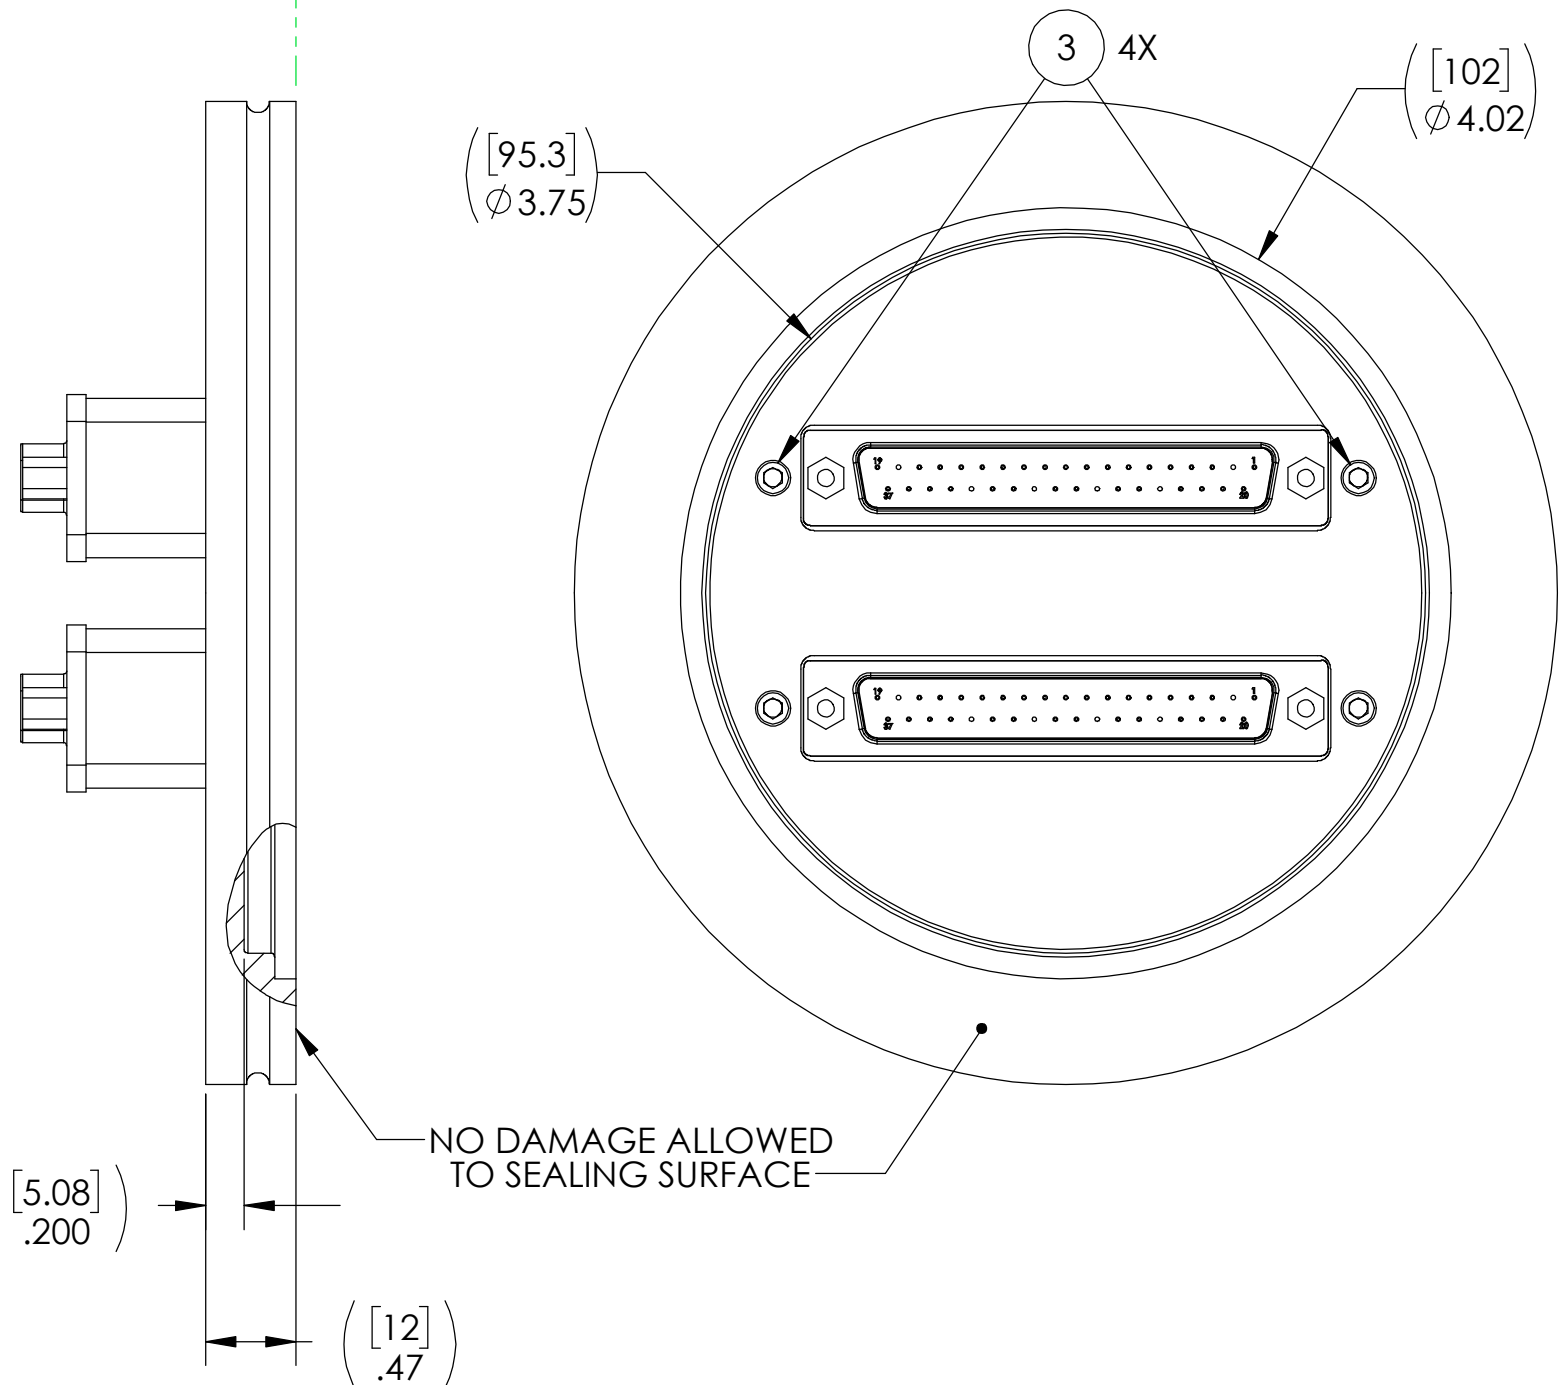

NOTES:

1. HE LEAK TEST @ 1 ATM. 1×10^{-6} CC/SEC OR LESS. A GREEN PAINT DOT ON THE ATMOSPHERE SIDE INDICATES THE ASSEMBLY HAS PASSED THE TEST.
2. ALCOHOL OR FOMBLIN YVAC 3 MAY BE USED TO LUBRICATE O-RINGS FOR VACUUM HELIUM LEAK TESTING.
3. ALL TESTS ARE PERFORMED AT ROOM TEMPERATURE.
4. ALL PARTS MUST PASS ALL TESTS.
5. SEE PAVE DRAWING# 6066 FOR INDIVIDUAL FEEDTHRU ASSEMBLY DETAILS INCLUDING ELECTRICAL TESTING.
6. REF-OPERATING TEMPERATURE RANGE -20°C TO 105°C.
7. DIMENSIONS ARE INCHES [millimeters].

ALL DIMENSIONS AND TOLERANCES APPLY TO FINISHED PART IN INCHES.
 ALLOWABLE TOLERANCES UNLESS SPECIFIED OTHERWISE: NONE ±0.5
 X.X DECIMAL ±0.1 X.XX DECIMAL ±0.02 X.XXX DECIMAL ±0.005
 ANGLES ±1 DEGREE SURFACE FINISH 128 microinch RMS

3	4	4-40X.3125 SHCS	SCREW SHCS 4-40x.3125-SS
2	2	6066R	SP58/13-E-150-37-K20-DSUB-DSUB
1	1	6067	FLANGE NW100-SS W/ 2X SP58/13 PORTS
ITEM	QTY	PART NUMBER	DESCRIPTION

		2751 Thunderhawk Court Dayton, OH 45414-3445 U.S.A. tel (937) 890-1100 fax (937) 8905165 www.pavetechnologyco.com	
DESCRIPTION			
FLANGE ASSEMBLY NW100-SS (2X) 6066R INSTALLED			
PART NUMBER	MATERIAL NOTED		
6062			
REVISION LEVEL	A	PROJECTION	